

01725625
FEB 05 2003
PATENT & TRADEMARK OFFICE

6599498

1/12


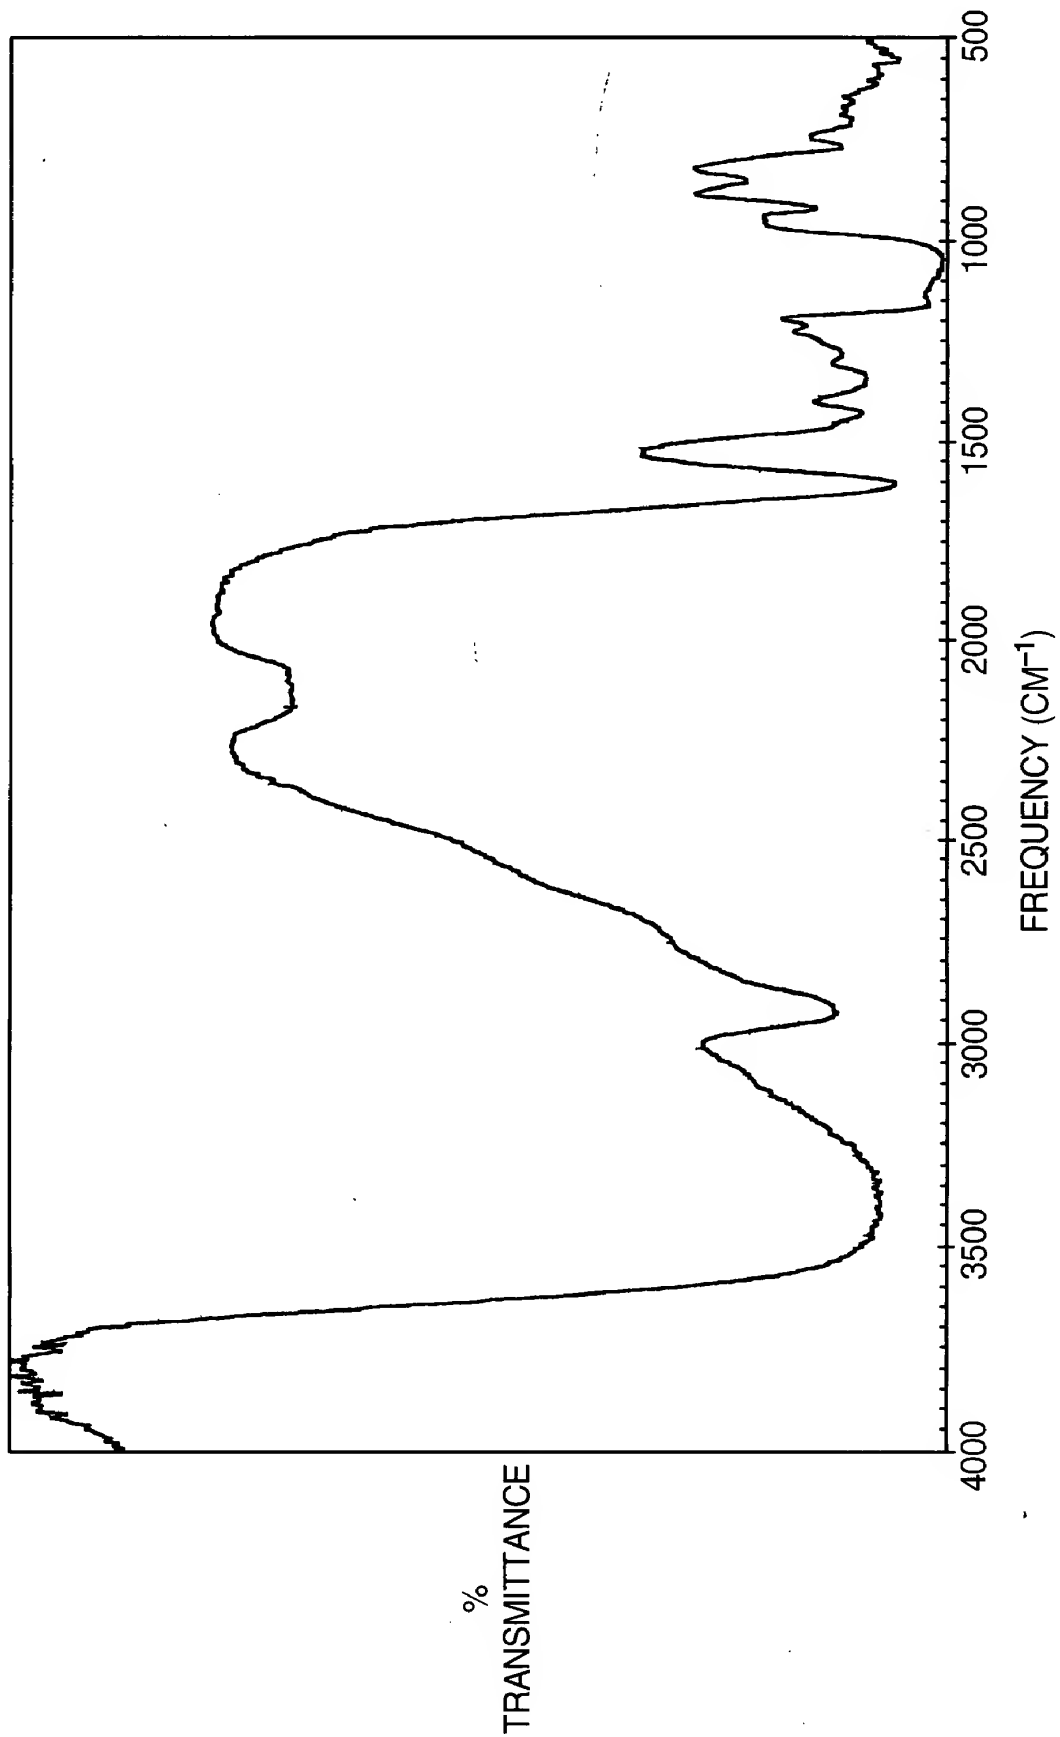


FIG. 1



2/12

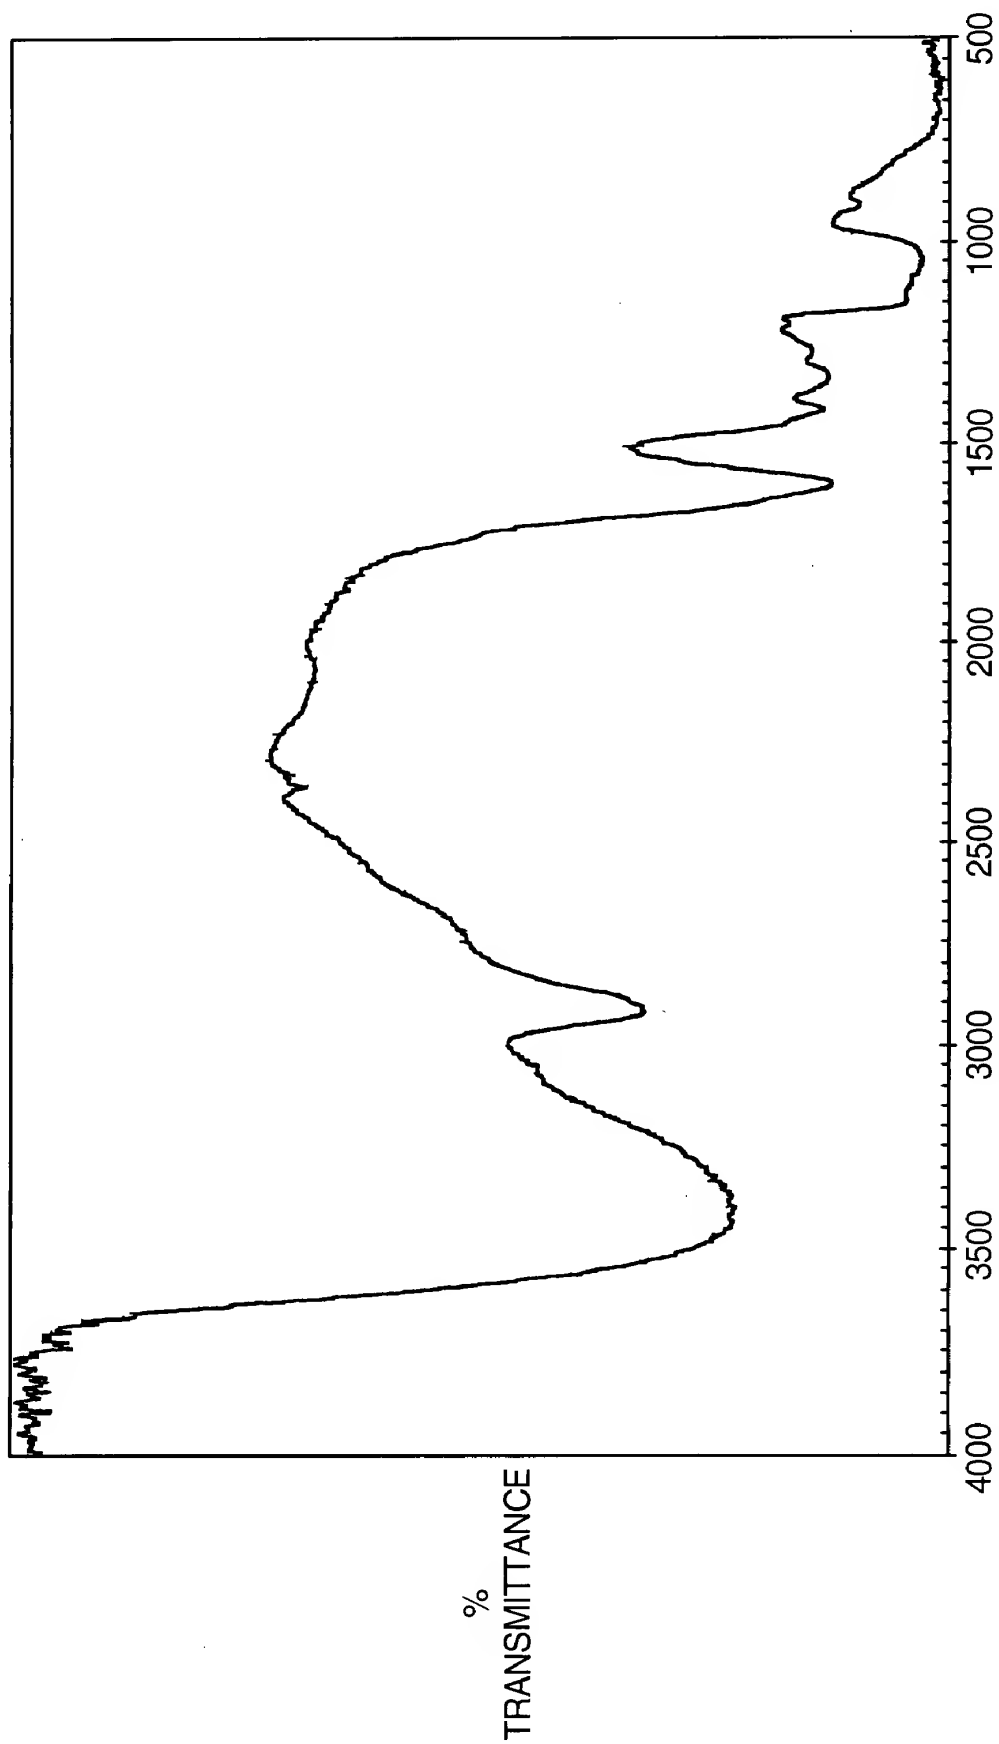

FREQUENCY (CM⁻¹)

FIG. 2



3/12


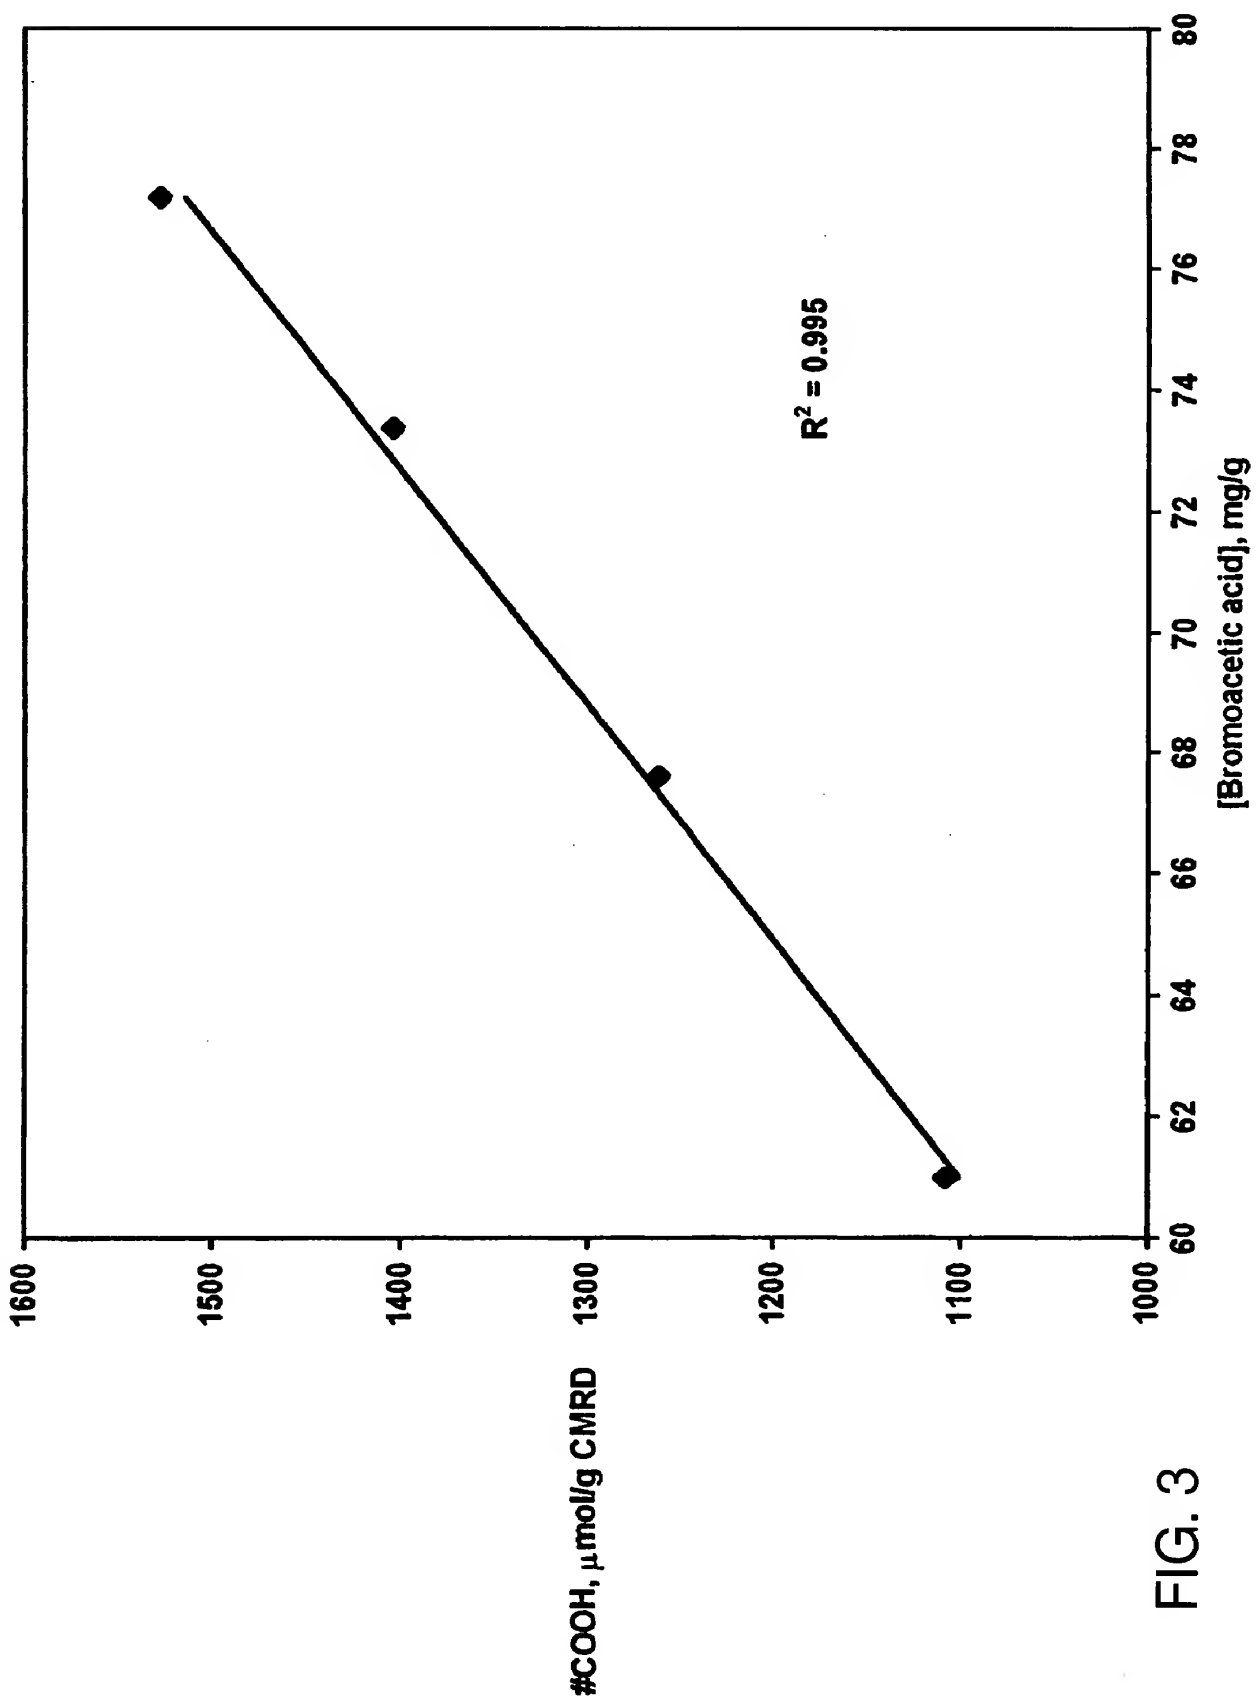


FIG. 3



4/12


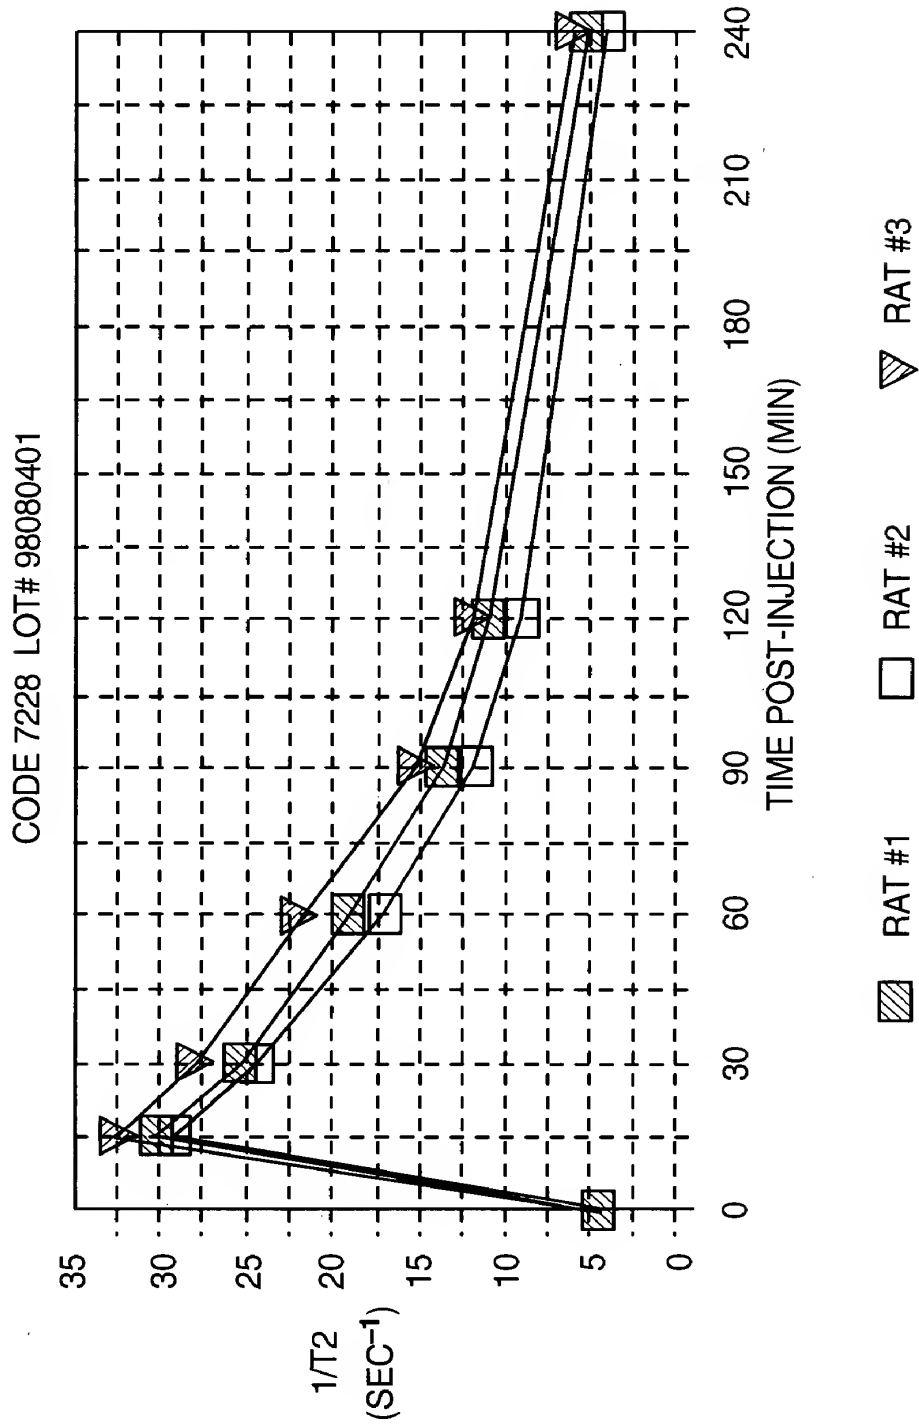


FIG. 4



5/12


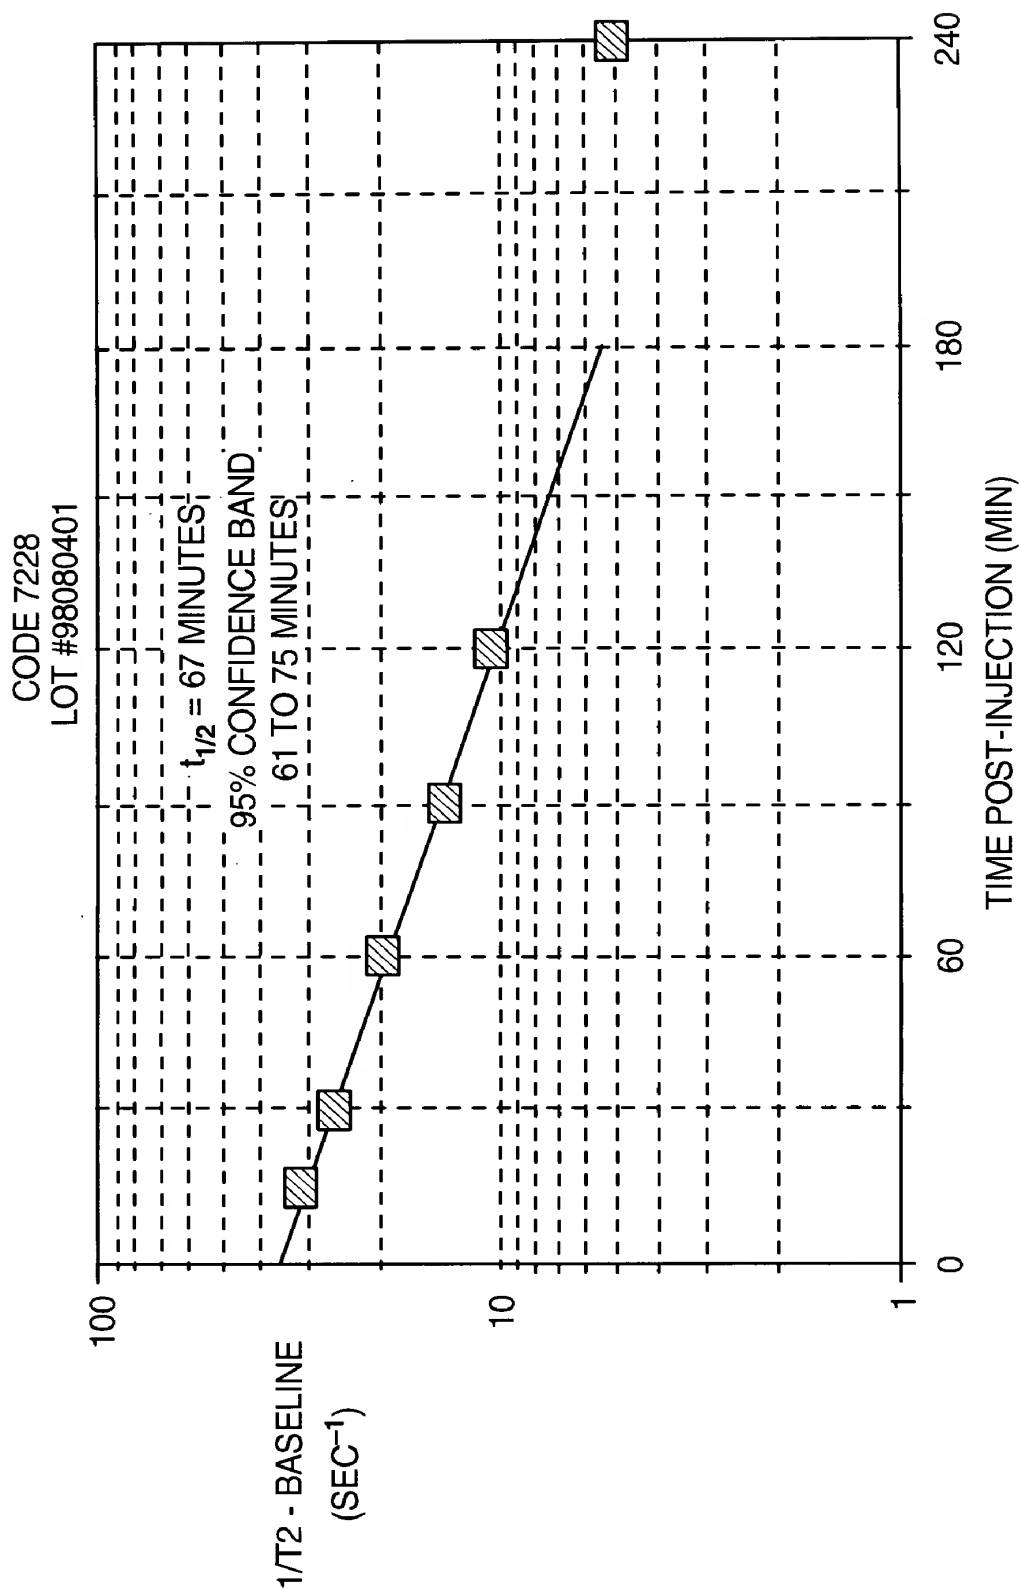


FIG. 5



6/12


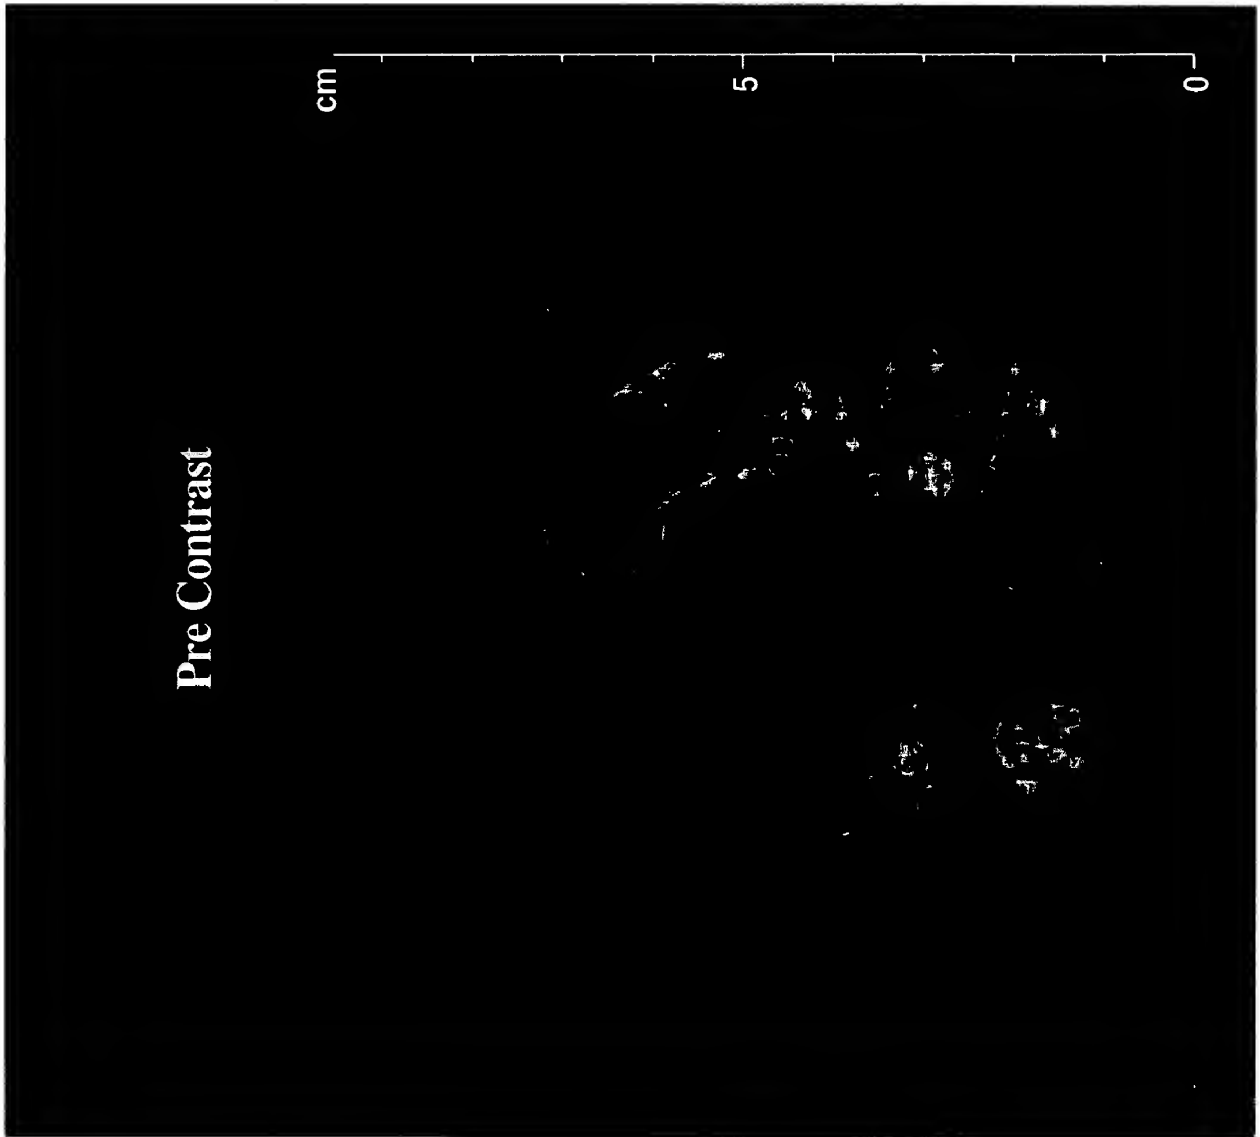


FIG. 6A



7/12

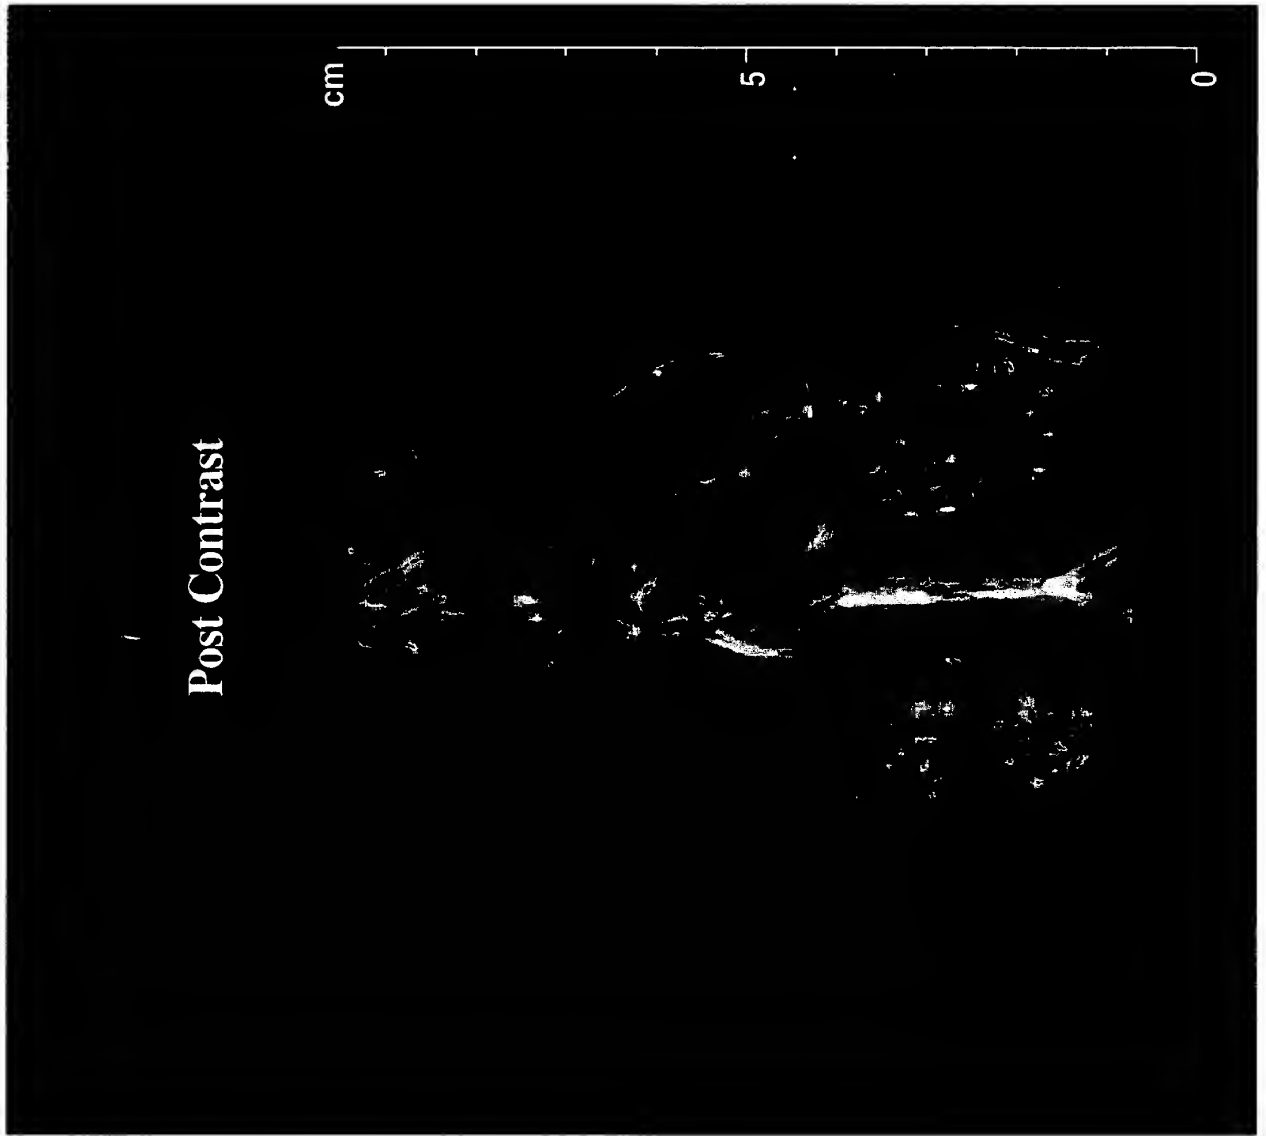

Post Contrast

FIG. 6B




8/12


Pre Contrast



FIG. 7A



9/12

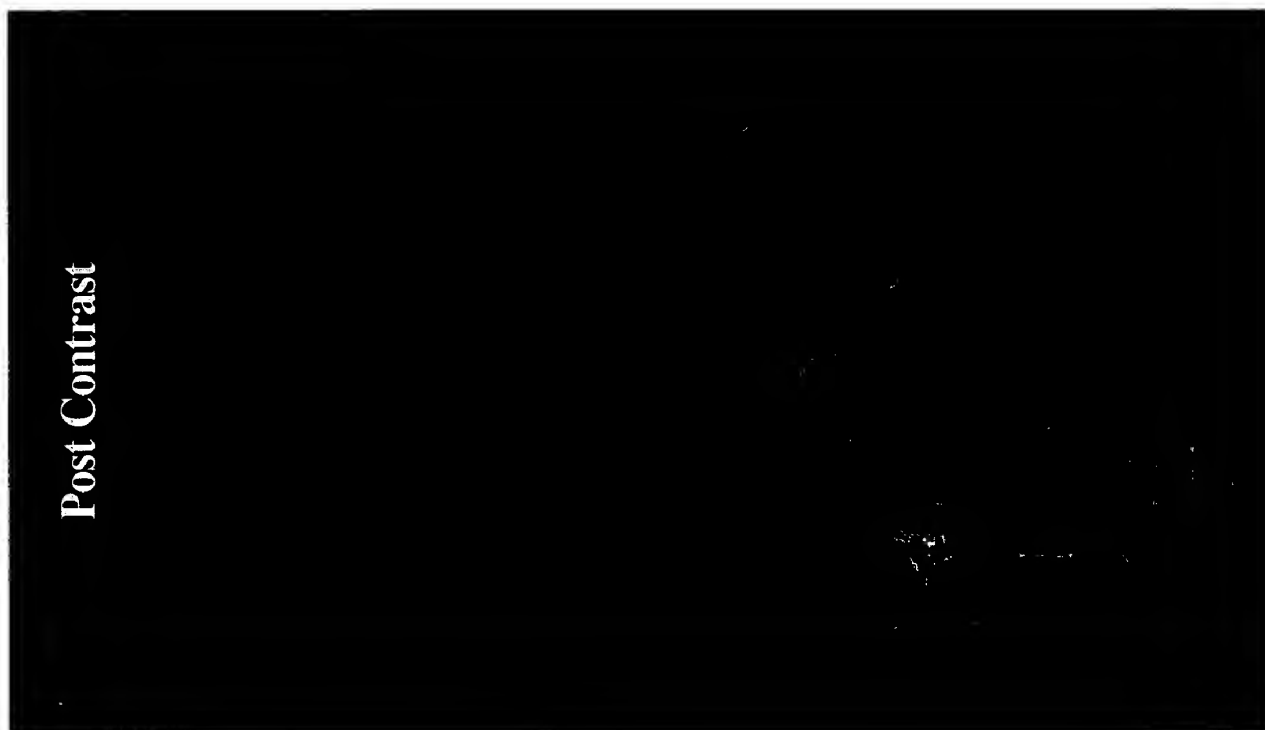


Post Contrast

FIG. 7B



10/12

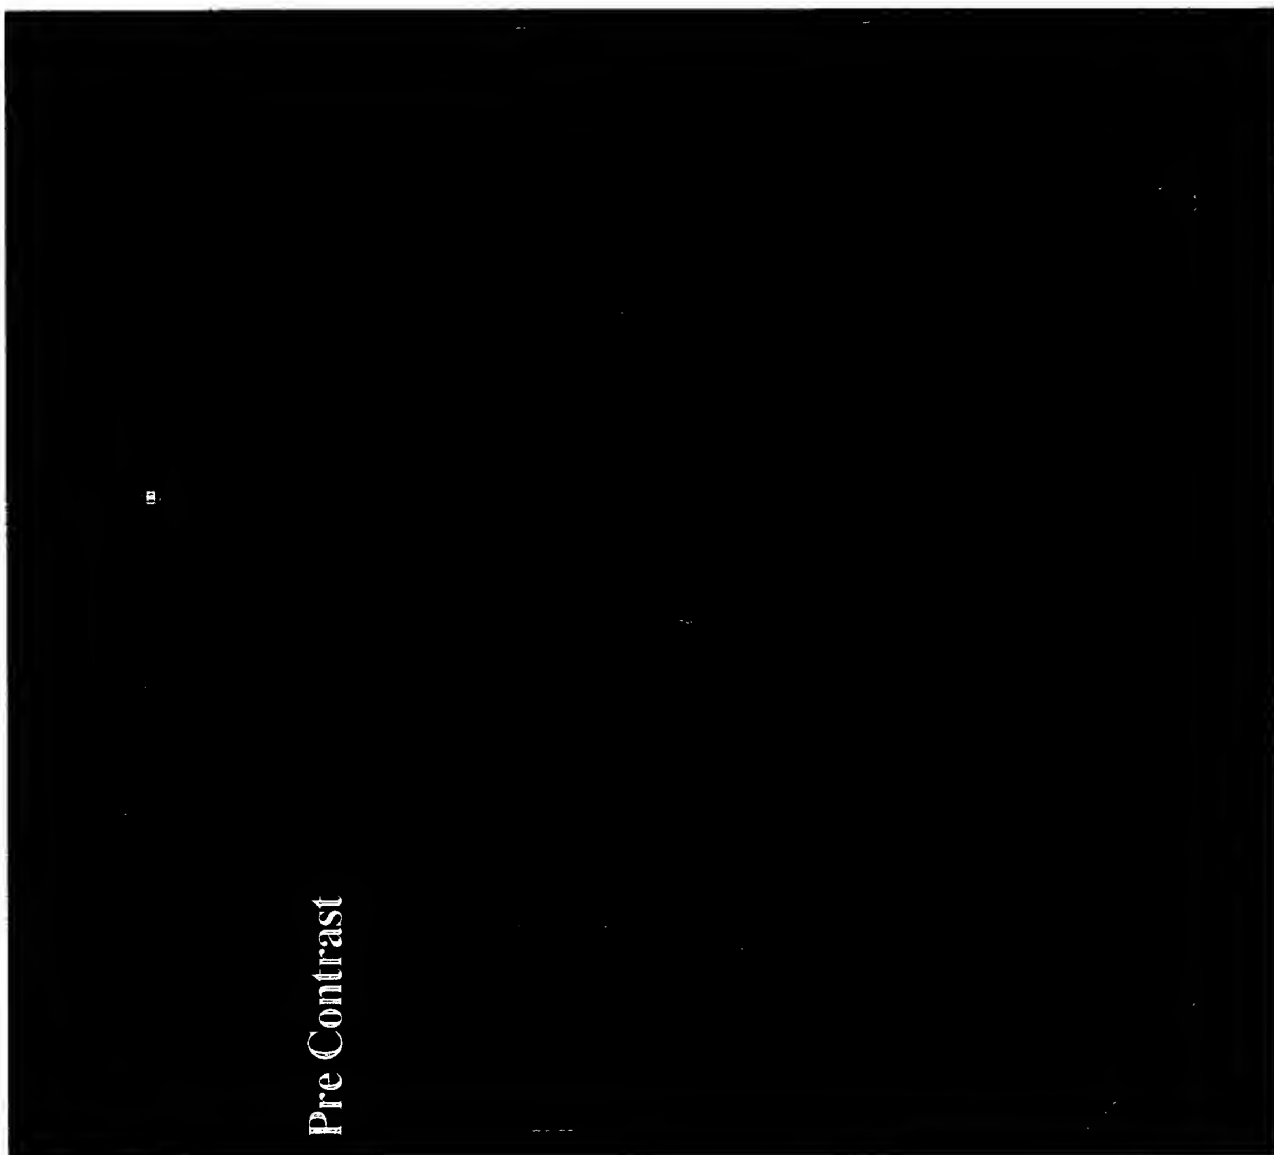

Pre Contrast


FIG. 8A



11/12



FIG. 8B



12/12

BLOOD CLEARANCE IN HUMANS AT 4 mg/kg

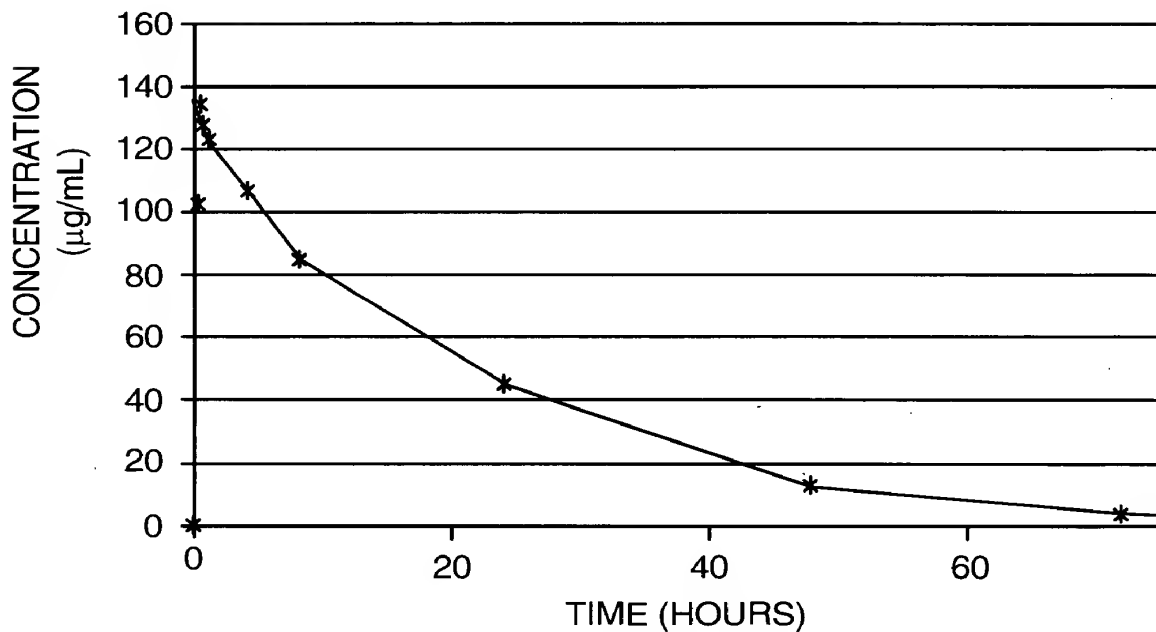


FIG. 9A

BLOOD CLEARANCE IN HUMANS AT 4 mg/kg

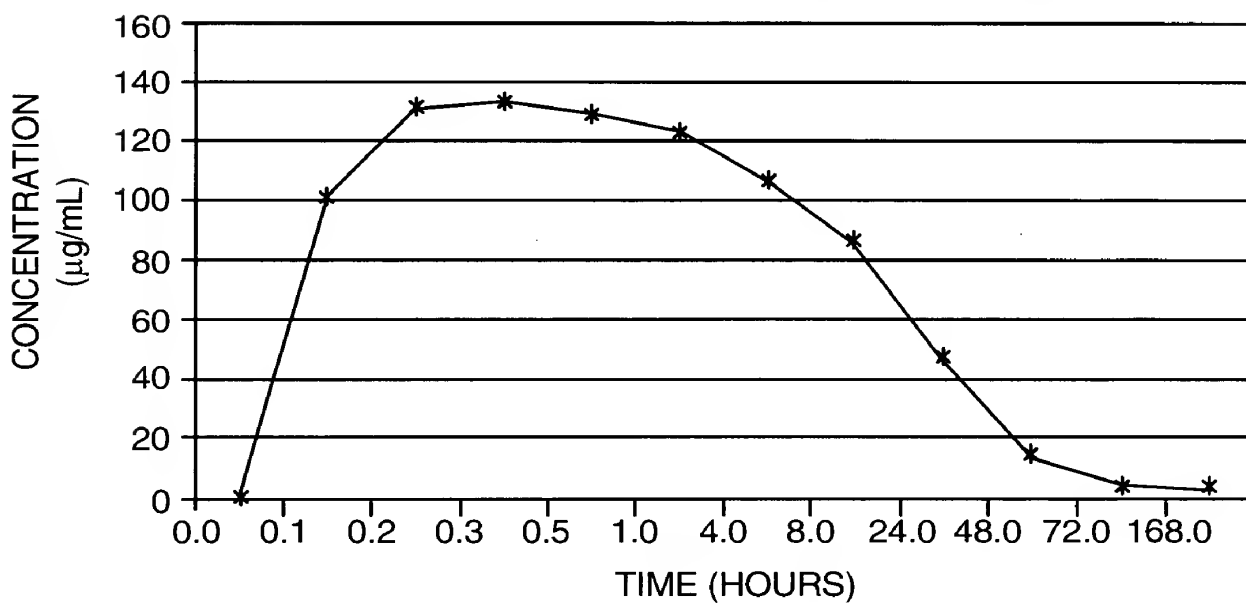


FIG. 9B